

BIOFIRE® PANELS

6 Panels. 170+ Targets. ~1 Hour.



BIOFIRE®
**RESPIRATORY 2.1 PLUS
PANEL**

23 Targets. ~45 Minutes.



BIOFIRE®
**BLOOD CULTURE
IDENTIFICATION 2 PANEL**

43 Targets. ~1 Hour.



BIOFIRE® FILMARRAY®
**GASTROINTESTINAL
PANEL**

22 Targets. ~1 Hour.



BIOFIRE® FILMARRAY®
**MENINGITIS/
ENCEPHALITIS PANEL**

14 Targets. ~1 Hour.



BIOFIRE® FILMARRAY®
PNEUMONIA PLUS PANEL

34 Targets. ~1 Hour.



BIOFIRE®
**JOINT INFECTION
PANEL**

39 Targets. ~1 Hour.



BIOFIRE® RESPIRATORY 2.1 PLUS (RP2.1plus) PANEL

23 Targets. ~45 Minutes.

VIRUSES

Adenovirus
Coronavirus 229E
Coronavirus HKU1
Coronavirus NL63
Coronavirus OC43
Middle East respiratory syndrome coronavirus (MERS-CoV)
Severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2)
Human metapneumovirus
Human rhinovirus/enterovirus

Influenza A virus
Influenza A virus A/H1
Influenza A virus A/H3
Influenza A virus A/H1-2009
Influenza B virus
Parainfluenza virus 1
Parainfluenza virus 2
Parainfluenza virus 3
Parainfluenza virus 4
Respiratory syncytial virus

BACTERIA

Bordetella parapertussis
Bordetella pertussis
Chlamydia pneumoniae
Mycoplasma pneumoniae



BIOFIRE RP2.1plus Panel Specifications

Sample Type: nasopharyngeal swab in transport media or saline

Hands-On Time: approximately 2 minutes

Sample Volume: 0.3 mL

Overall Performance: 97.1% sensitivity, 99.3% specificity¹
SARS-CoV-2 Performance: 98.4% PPA, 98.9% NPA²

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE RP2.1plus Panel Reagent Kit (30 Pouches): 423740

1. Overall performance based on prospective clinical study for the BIOFIRE® FILMARRAY® Respiratory 2 plus Panel, data on file, BioFire Diagnostics.

2. Overall performance based on prospective SARS-CoV-2 clinical study for the BIOFIRE® Respiratory 2.1 plus Panel in comparison to 3 EUA tests, data on file, BioFire Diagnostics.



BIOFIRE® BLOOD CULTURE IDENTIFICATION 2 (BCID2) PANEL

43 Targets. ~1 Hour.

GRAM-NEGATIVE BACTERIA

*Acinetobacter calcoaceticus-
baumannii* complex
Bacteroides fragilis
Enterobacterales
 Enterobacter cloacae complex
 Escherichia coli
 Klebsiella aerogenes
 Klebsiella oxytoca
 Klebsiella pneumoniae group
 Proteus spp.
 Salmonella spp.
 Serratia marcescens
Haemophilus influenzae
Neisseria meningitidis
Pseudomonas aeruginosa
Stenotrophomonas maltophilia

GRAM-POSITIVE BACTERIA

Enterococcus faecalis
Enterococcus faecium
Listeria monocytogenes
Staphylococcus spp.
 Staphylococcus aureus
 Staphylococcus epidermidis
 Staphylococcus lugdunensis
Streptococcus spp.
 Streptococcus agalactiae
 Streptococcus pneumoniae
 Streptococcus pyogenes

YEAST

Candida albicans
Candida auris
Candida glabrata
Candida krusei
Candida parapsilosis
Candida tropicalis
Cryptococcus (*C. neoformans*/*C. gattii*)

ANTIMICROBIAL RESISTANCE GENES

Carbapenemases

IMP
KPC
OXA-48-like
NDM
VIM

Colistin Resistance

mcr-1

ESBL

CTX-M

Methicillin Resistance

mecA/C
mecA/C and MREJ (MRSA)

Vancomycin Resistance

vanA/B

FDA cleared |  2797

BIOFIRE BCID2 Panel Specifications

Sample Type: positive blood culture

Hands-On Time: approximately 2 minutes

Sample Volume: 0.2 mL

Performance: 99.0% sensitivity, 99.8% specificity³

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE BCID2 Panel Reagent Kit (30 Pouches): RFIT-ASY-0147

3. Overall performance is the aggregate of the prospective, archived, and seeded data from the clinical studies. Data on file, BioFire Diagnostics.



BIOFIRE® FILMARRAY® GASTROINTESTINAL (GI) PANEL

22 Targets. ~1 Hour.

BACTERIA

Campylobacter (*C. jejuni*/*C. coli*/*C. upsaliensis*)
Clostridioides (*Clostridium*) *difficile* (toxin A/B)*
Plesiomonas shigelloides
Salmonella
Vibrio (*V. parahaemolyticus*/*V. vulnificus*/*V. cholerae*)
Vibrio cholerae
Yersinia enterocolitica
Diarrheagenic *Escherichia coli*/*Shigella*
Enteroaggregative *E. coli* (EAEC)
Enteropathogenic *E. coli* (EPEC)
Enterotoxigenic *E. coli* (ETEC) *lt/st*
Shiga-like toxin-producing *E. coli* (STEC) *stx1/stx2*
E. coli O157
Shigella/Enteroinvasive *E. coli* (EIEC)

*Selective reporting available for *C. diff*

VIRUSES

Adenovirus F40/41
Astrovirus
Norovirus GI/GII
Rotavirus A
Sapovirus (I, II, IV, and V)

PARASITES

Cryptosporidium
Cyclospora cayetanensis
Entamoeba histolytica
Giardia lamblia

FDA cleared | CE₂₇₉₇

BIOFIRE GI Panel Specifications

Sample Type: stool sample in Cary Blair

Hands-On Time: approximately 2 minutes

Sample Volume: 0.2 mL

Performance: 98.5% sensitivity, 99.2% specificity⁴

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE GI Panel Reagent Kit (30 Pouches): RFIT-ASY-0116

BIOFIRE GI Panel Reagent Kit (6 Pouches): RFIT-ASY-0104

4. Overall performance based on prospective clinical study for the BIOFIRE® FILMARRAY® Gastrointestinal Panel, data on file, BioFire Diagnostics.



BIOFIRE® FILMARRAY® MENINGITIS/ENCEPHALITIS (ME) PANEL

14 Targets. ~1 Hour.

BACTERIA

Escherichia coli K1
Haemophilus influenzae
Listeria monocytogenes
Neisseria meningitidis
Streptococcus agalactiae
Streptococcus pneumoniae

VIRUSES

Cytomegalovirus (CMV)
Enterovirus (EV)
Herpes simplex virus 1 (HSV-1)
Herpes simplex virus 2 (HSV-2)
Human herpesvirus 6 (HHV-6)
Human parechovirus (HPeV)
Varicella zoster virus (VZV)

YEAST

Cryptococcus (C. neoformans/C. gattii)

FDA cleared | CE₂₇₉₇

BIOFIRE ME Panel Specifications

Sample Type: cerebrospinal fluid (CSF)

Hands-On Time: approximately 2 minutes

Sample Volume: 0.2 mL

Performance: 94.2% sensitivity, 99.8% specificity⁵

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE ME Panel Reagent Kit (30 Pouches): RFIT-ASY-0118

BIOFIRE ME Panel Reagent Kit (6 Pouches): RFIT-ASY-0119

5. Overall performance based on prospective clinical study for the BIOFIRE® FILMARRAY® Meningitis/Encephalitis Panel, data on file, BioFire Diagnostics.



BIOFIRE® FILMARRAY® PNEUMONIA *PLUS* (PN*plus*) PANEL

34 Targets. ~1 Hour.

BACTERIA (Semi-Quantitative)

Acinetobacter calcoaceticus-
baumannii complex
Enterobacter cloacae complex
Escherichia coli
Haemophilus influenzae
Klebsiella aerogenes
Klebsiella oxytoca
Klebsiella pneumoniae group
Moraxella catarrhalis
Proteus spp.
Pseudomonas aeruginosa
Serratia marcescens
Staphylococcus aureus
Streptococcus agalactiae
Streptococcus pneumoniae
Streptococcus pyogenes

ATYPICAL BACTERIA (Qualitative)

Chlamydia pneumoniae
Legionella pneumophila
Mycoplasma pneumoniae

VIRUSES

Adenovirus
Coronavirus
Human metapneumovirus
Human rhinovirus/enterovirus
Influenza A virus
Influenza B virus
Middle East respiratory syndrome
coronavirus (MERS-CoV)
Parainfluenza virus
Respiratory syncytial virus

ANTIMICROBIAL RESISTANCE GENES

Carbapenemases

IMP
KPC
NDM
OXA-48-like
VIM

ESBL CTX-M

Methicillin Resistance *mecA/C* and MREJ (MRSA)



BIOFIRE PN*plus* Panel Specifications

Sample Type: BAL-like (including mini-BAL), Sputum-like (including ETA)

Hands-On Time: approximately 2 minutes

Performance: BAL-like (including mini-BAL): 96.2% sensitivity, 98.4% specificity; Sputum-like (including ETA): 96.3% sensitivity, 97.3% specificity⁶

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE PN*plus* Panel Reagent Kit (30 Pouches): RFIT-ASY-0143

6. Overall performance based on prospective clinical study for the BIOFIRE® FILMARRAY® Pneumonia *plus* Panel, data on file, BioFire Diagnostics.



BIOFIRE® JOINT INFECTION (JI) PANEL

39 Targets. ~1 Hour.

GRAM-POSITIVE BACTERIA

Anaerococcus prevotii/vaginalis
Clostridium perfringens
Cutibacterium avidum/granulosum
Enterococcus faecalis
Enterococcus faecium
Fingoldia magna
Parvimonas micra
Peptoniphilus
Peptostreptococcus anaerobius
Staphylococcus aureus
Staphylococcus lugdunensis
Streptococcus spp.
Streptococcus agalactiae
Streptococcus pneumoniae
Streptococcus pyogenes

GRAM-NEGATIVE BACTERIA

Bacteroides fragilis
Citrobacter
Enterobacter cloacae complex
Escherichia coli
Haemophilus influenzae
Kingella kingae
Klebsiella aerogenes
Klebsiella pneumoniae group
Morganella morganii
Neisseria gonorrhoeae
Proteus spp.
Pseudomonas aeruginosa
Salmonella spp.
Serratia marcescens

YEAST

Candida spp.
Candida albicans

ANTIMICROBIAL RESISTANCE GENES

Carbapenemases

IMP
KPC
NDM
OXA-48-like
VIM

ESBL

CTX-M

Methicillin Resistance

mecA/C and MREJ (MRSA)

Vancomycin Resistance

vanA/B

FDA cleared | CE₂₇₉₇

BIOFIRE JI Panel Specifications

Sample Type: synovial fluid

Hands-On Time: approximately 2 minutes

Sample Volume: 0.2 mL


Performance: 91.7% sensitivity, 99.8% specificity⁷

Storage Conditions: all kit components stored at room temperature (15-25 °C)

Part Number

BIOFIRE JI Panel Reagent Kit (30 Pouches): RFIT-ASY-0138

7. Overall performance based on prospective clinical study for the BIOFIRE® Joint Infection Panel, data on file, BioFire Diagnostics.

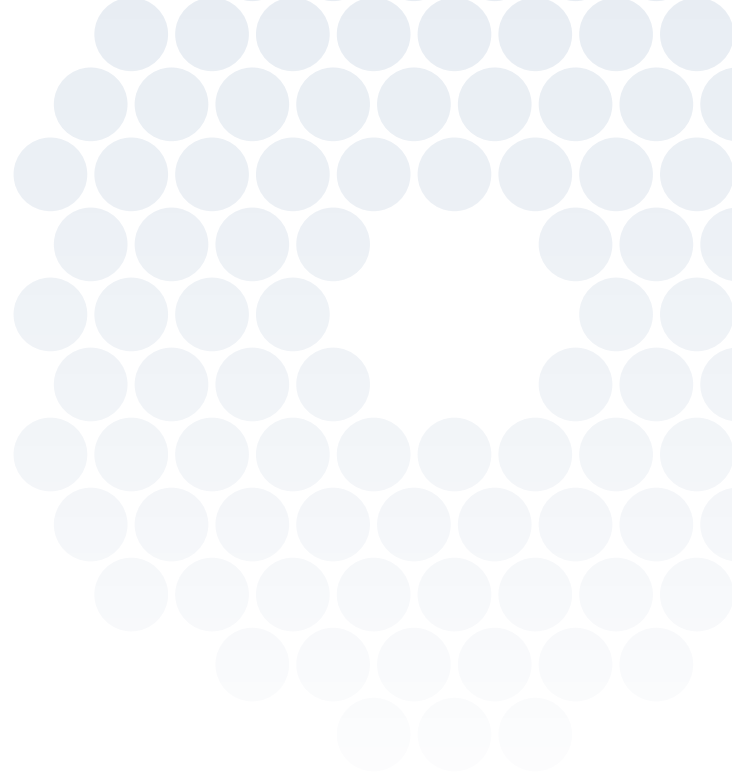

Scan the QR code
for more information.

Learn more about the BIOFIRE range of commercially-available
panels for syndromic infectious disease diagnostics.



Contact Us

bioMérieux S.A.
69280 Marcy l'Etoile
France
Tel: +33 (0) 4 78 87 20 00
Fax: +33 (0) 4 78 87 20 90
biomerieux.com

Manufactured by:
BioFire Diagnostics, LLC
515 Colorow Drive
Salt Lake City, UT 84108 USA
Tel: +1-801-736-6354
biofiredx.com

Product availability varies by country. Consult your bioMérieux representative.

9325496 007/GB/C BFR001-3801-04